



REPLACEMENT SHEET
TITLE: "BLOOD SAMPLING DEVICE"
SERIAL No.: 10/737,016
ATTY: BRADLEY K. GROFF
ATTY TEL: 770.984.2300
ATTY DOCKET No.: 2G02.1-080

16/35

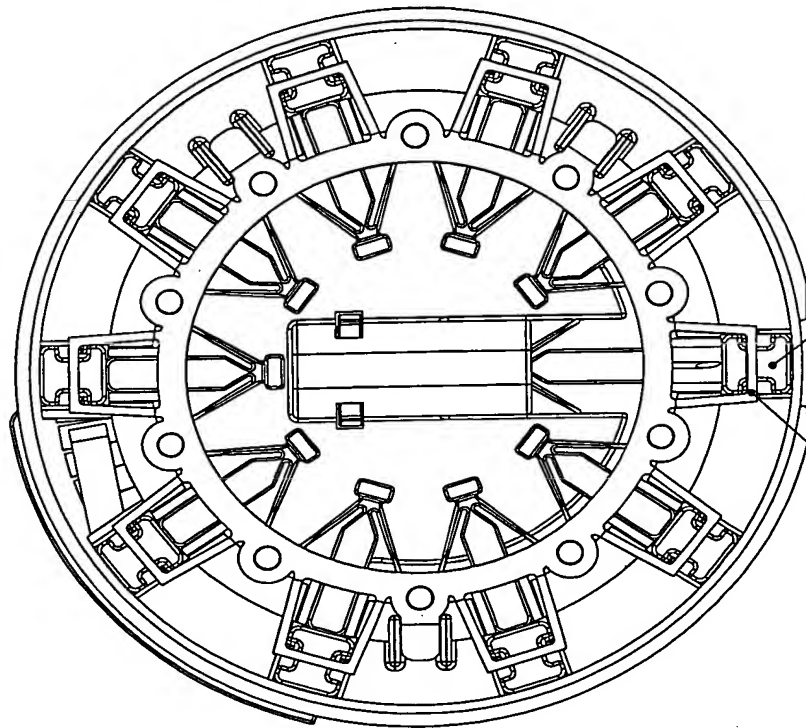


FIG. 26B

174
176

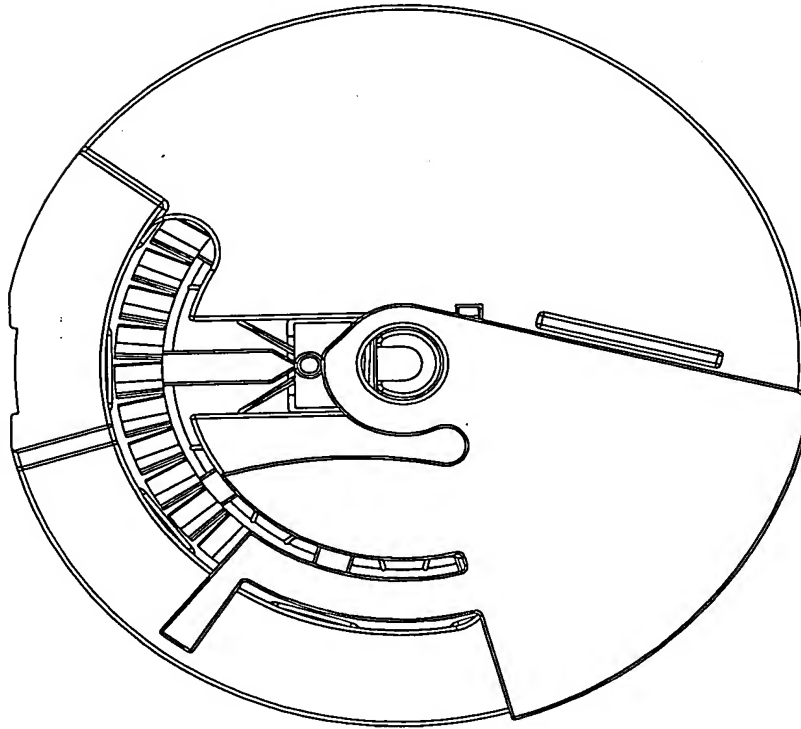


FIG. 26A

18/35

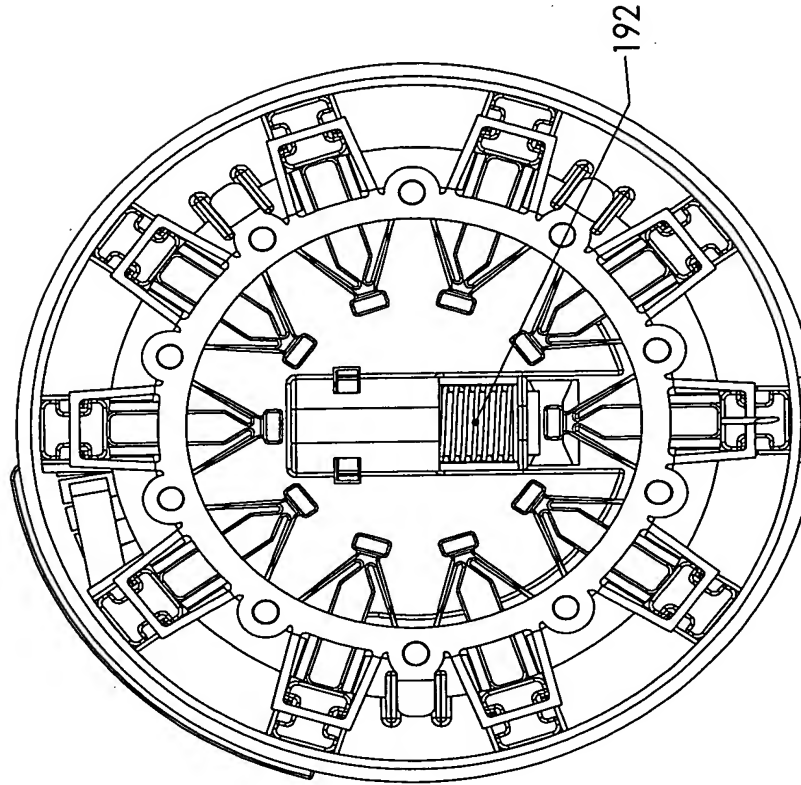


FIG. 28B

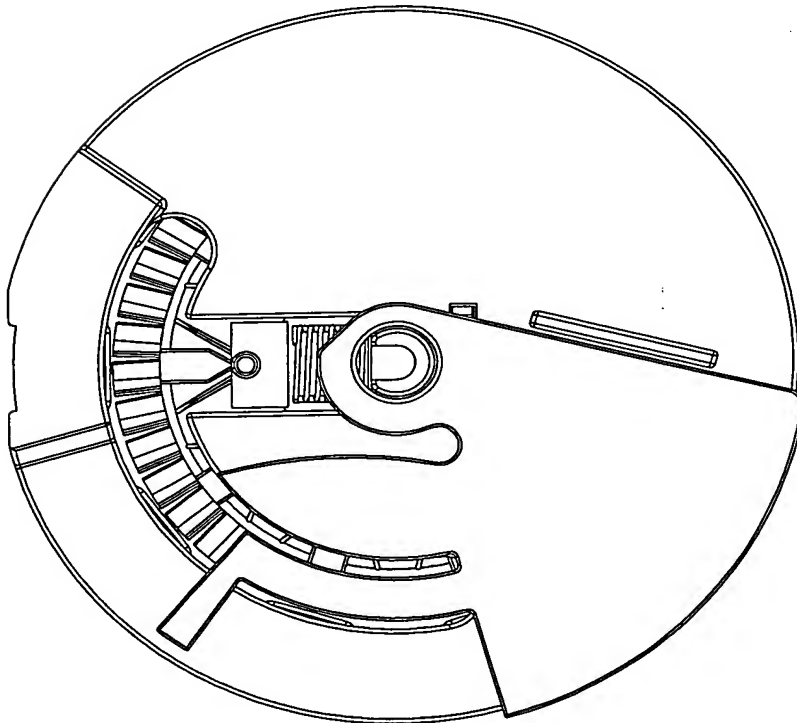


FIG. 28A

24/35

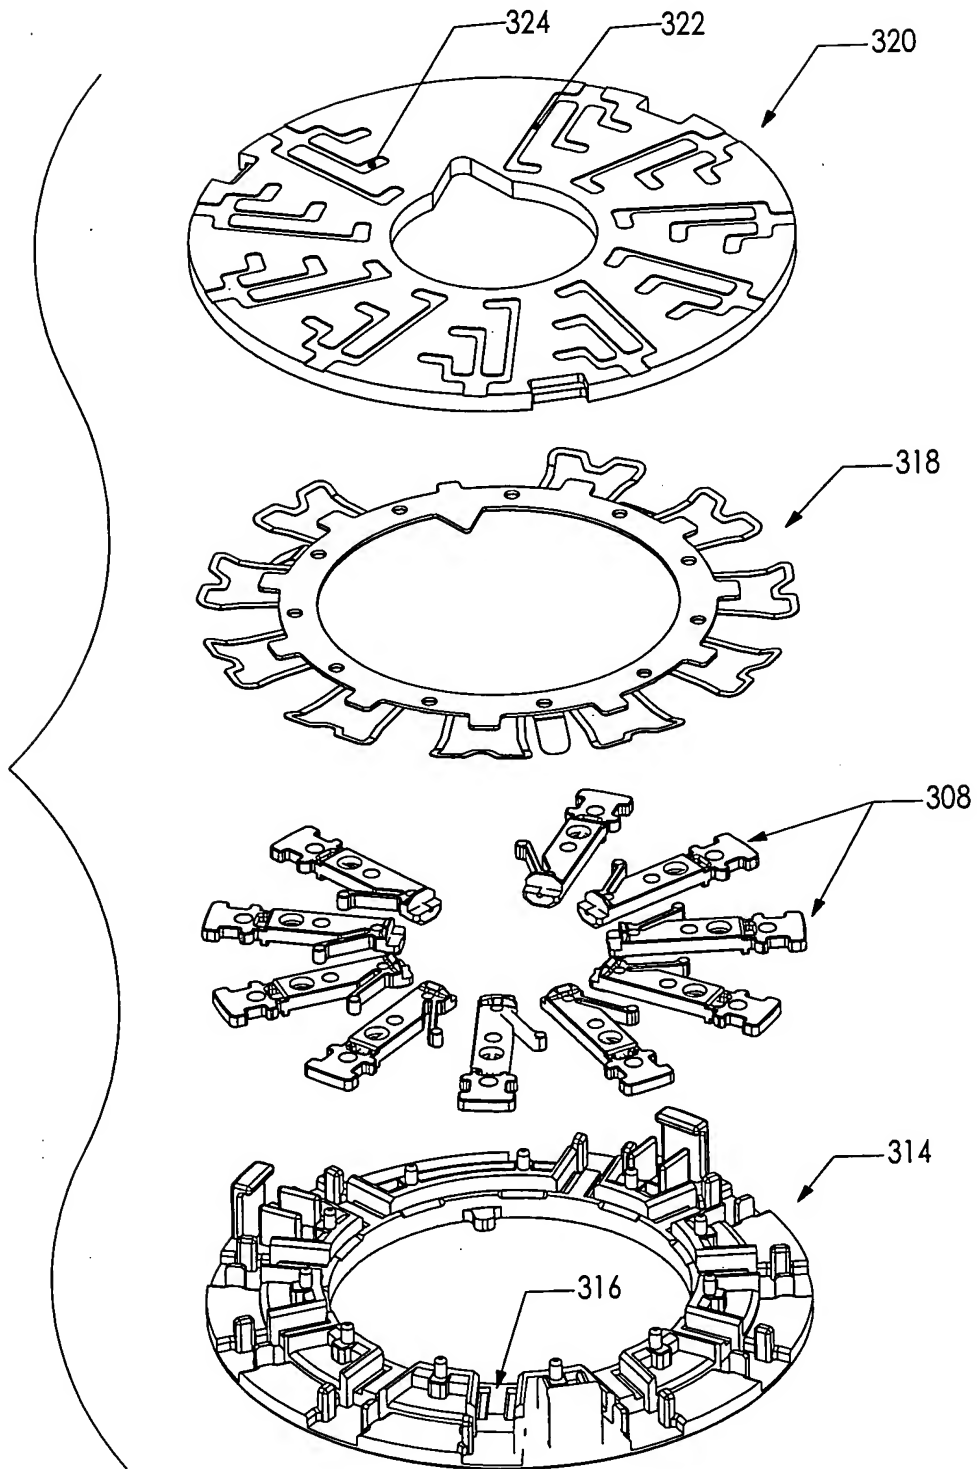


FIG. 35